

# A LASER-POLYMERIZED THIN FILM SILICA SURFACE MODIFICATION FOR SUPPRESSION OF CELL ADHESION AND ELECTROSMOTIC FLOW IN MICROCHANNELS

Brian J. Kirby<sup>1</sup>, Aaron R. Wheeler<sup>2</sup>, Timothy J. Shepodd<sup>1</sup>,  
Julia A. Fruetel<sup>1</sup>, Ernest F. Hasselbrink<sup>1</sup>, Richard N. Zare<sup>2</sup>

<sup>1</sup> Sandia National Laboratories, PO Box 969, Livermore, CA 94551-0969

<sup>2</sup> Chemistry Department, Stanford University, Stanford, CA

## Abstract

A laser-polymerized thin film for silica surface modification is presented. This technique enables photopatterned surface charge modification consistent with optical tweezer techniques. This charge modification may be applied for chip-based cell techniques and multi-dimensional separation techniques that require nonuniform zeta potential on a microfluidic chip.

**Keywords:** surface modification, zeta potential, cell adhesion

## 1. Introduction

Silica surface charge interferes with a number of microfluidic chip-based techniques (*e.g.*, capillary isoelectric focusing (cIEF)) by inducing unwanted electroosmotic flow (EOF); this surface charge can also interfere with chip-based cell techniques by causing cells to electrostatically adhere to cell walls. Two-dimensional separations may require selectively eliminating zeta potential ( $\zeta$ ) on one part of a microfluidic chip while  $\zeta$  is retained in other sections. Use of optical tweezers for cell manipulation on-chip [1] further requires that surface modifications be nonabsorbent and nonscattering at the laser wavelength.

## 2. Surface Modification Mechanism

An aqueous mixture of 3-(trimethoxysilyl)-propyl acrylate (Aldrich) and acetic acid is applied to pretreat the silica surface (Figure 1), covalently bonding the acrylate intermediary to exposed surface charge sites. This intermediary affects  $\zeta$  only slightly, and hence does not inhibit electroosmotic flow. Following this pre-treatment, frequency-tripled Nd:YAG laser emission (355 nm) is used to locally polymerize acrylamide to the intermediary. Flushing the solution leaves a photopatterned acrylamide thin film.

## 3. Measurements

Streaming potential was used to measure  $\zeta$  in silica capillaries with and without surface modifications. For 1 mM phosphate buffer solutions (K<sup>+</sup> cation, pH 7.3 +/- 0.2),  $\zeta$  was measured at -83 +/- 3 mV, -75 +/- 3 mV, and 0 +/- 1 mV for untreated, pretreated, and polymerized surfaces, respectively; the photopatterned polyacrylamide thin film

creates an uncharged ( $\zeta=0$ ) surface but the pretreat step does not significantly affect  $\zeta$ . A solution containing murine bone marrow mast cells ( $d=10\ \mu\text{m}$ ), glucose, and phosphate buffer was brought into contact with untreated and polymerized silica surfaces on glass cover slides and a wet-etched glass chip ( $30 \times 150\ \mu\text{m}$  channels). Cell adhesion was inferred from images after flushing with solution. On cover slides, cells appear post-flush only if adhered to the surface (Figure 2). In microchannels, adhered cells appear the same regardless of flow rate, while cells in the bulk appear only as a faint background in the flowing image. Figure 3 shows cell solutions in microchannels with and without flow (flowrates as high as  $20\ \text{cm/s}$  were used). The polyacrylamide thin film prevents mast cell adhesion.

## References

1. A.R. Wheeler, K. Morishima, D.W. Arnold, A.B. Rossi, and R.N. Zare, Single Organelle Analysis with Integrated Chip Electrophoresis and Optical Tweezers, in *Micro Total Analysis Systems 2000*, A. van den Berg et al. (eds.), (2000).

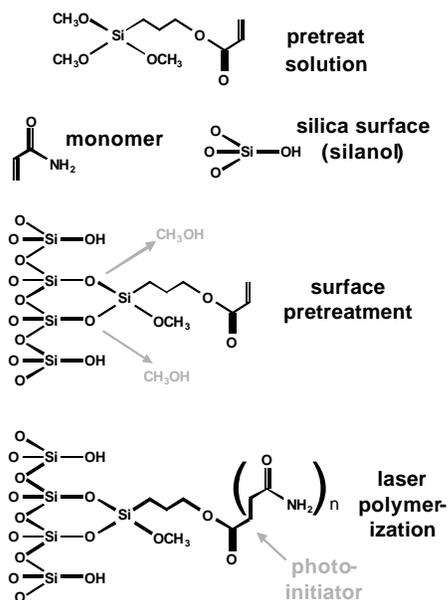


Figure 1. Surface pretreatment and laser-polymerization steps.

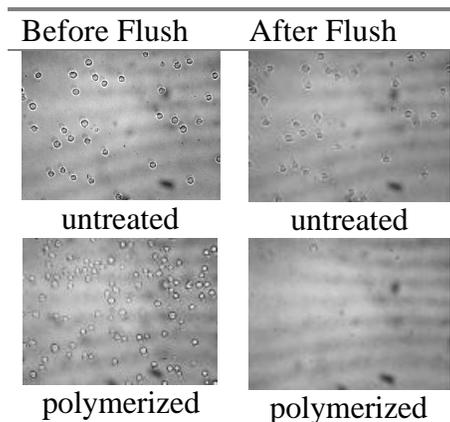


Figure 2. Cell adhesion on cover slides.

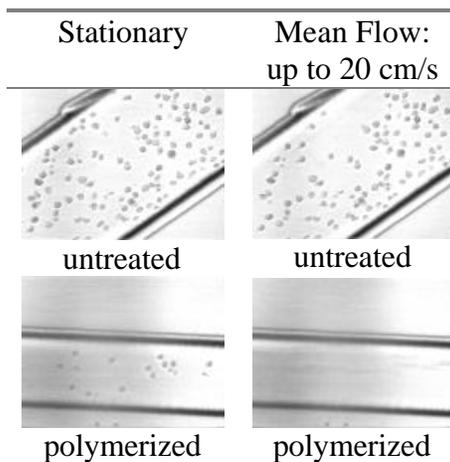


Figure 3. Cell adhesion in glass microchannels.